CIRCLING APPROACH CHART

ELEV 915 ft (279 m)

ATIS	**121.175**		
TWR	**120.250**	**119.700**	**121.500**
CLR DEL	**121.780**		

LUGANO
DAY ONLY
CIRCLING FOXTROT
RWY 19

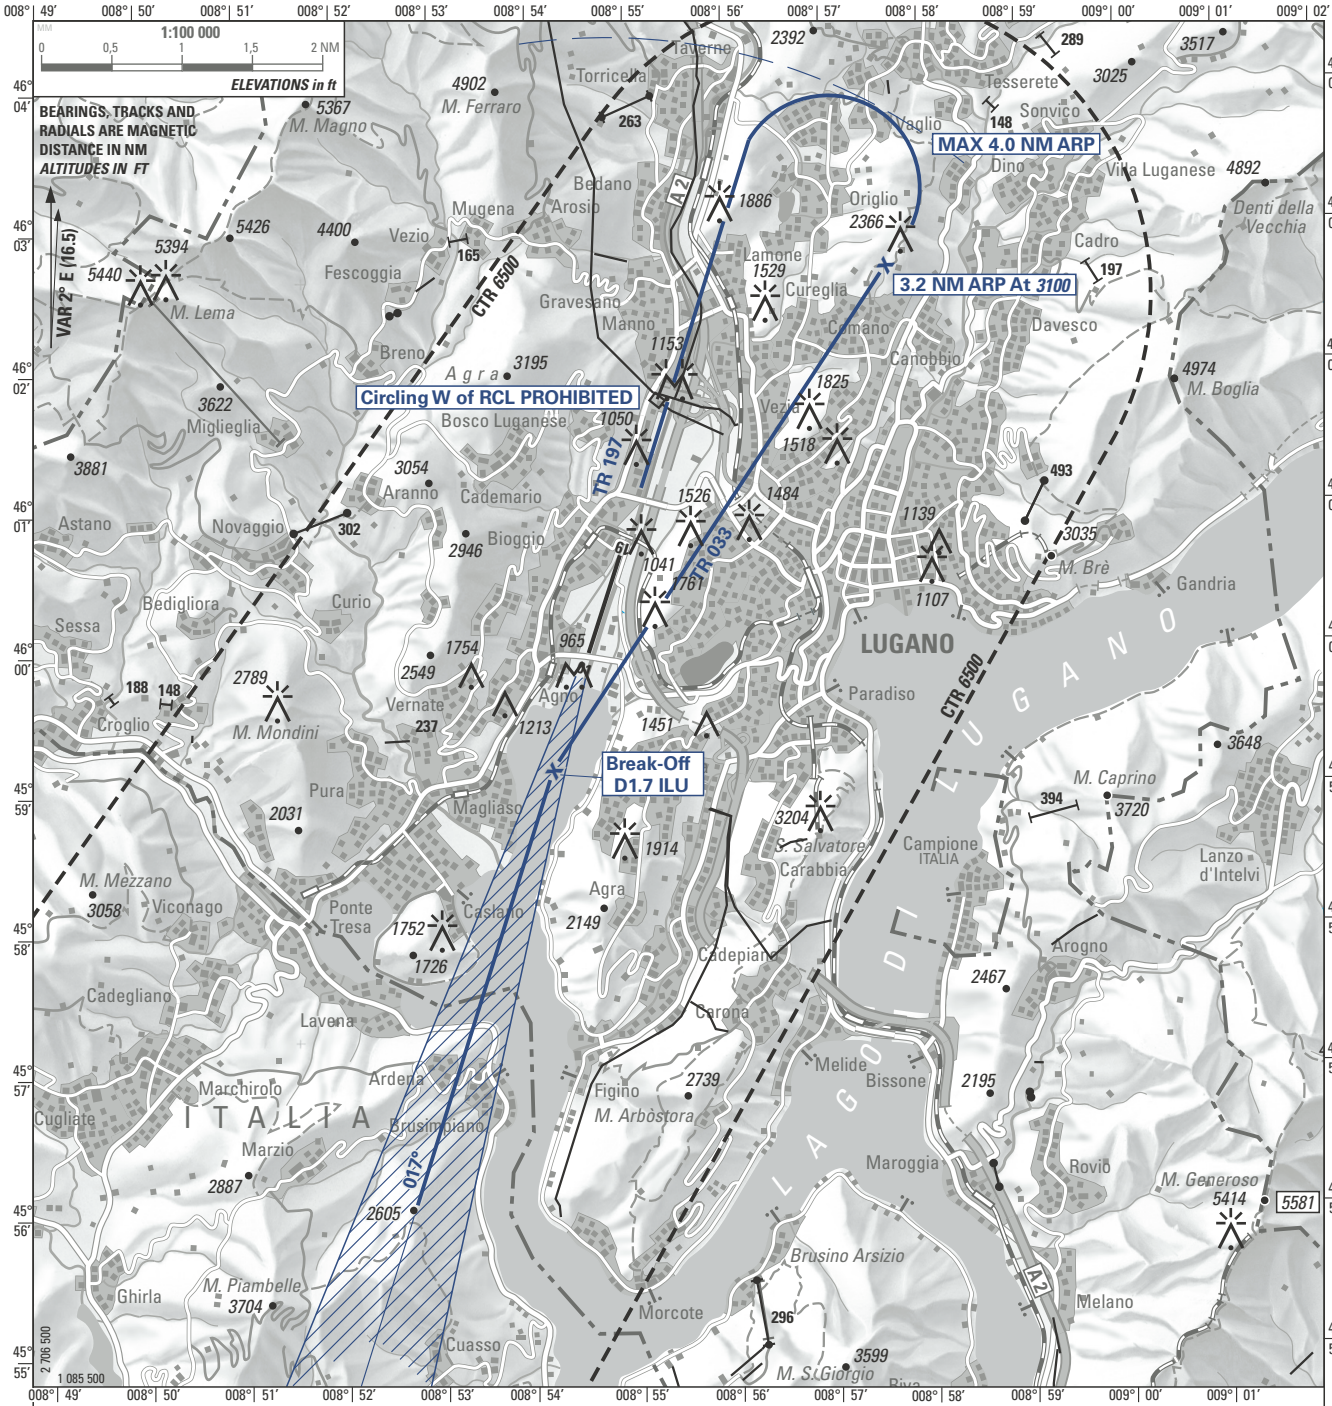

WARNING: Disregard PAPI RWY 01 information.
Use PAPI RWY 19 information only within 2 NM from THR

Descent to be arranged to maintain clean configuration as long as possible, safety and ATC requirement considered.

OBST ELEV: *ft* / HGT: **ft**

OCA/H CIRCLING A & B	VIS m	CEILING REQUIRED
3100 (2185) *3500* (2585) if ceiling and VIS permit	Day only 5000	3100 ft AAL or higher

CIRCLING PROCEDURE

If visual contact is established at D2.2 ILU, continue straight ahead. At D1.7 ILU turn right on track 033°, if ceiling and visibility permit maintain *3500 ft* for noise abatement purposes (*3100 ft* procedure MNM) until 3.2 NM ARP.

At 3.2 NM ARP start left turn onto base.

COR: OBST, editorial (WEF 13JUL2023)

© swisstopo

THIS PAGE INTENTIONALLY LEFT BLANK